

Results History


The information provided below is in the electronic medical record. If you believe any data is incorrect, please notify your healthcare provider.

GORDON WATTS

PSA
(ng/mL)

Time
Range

1 day 

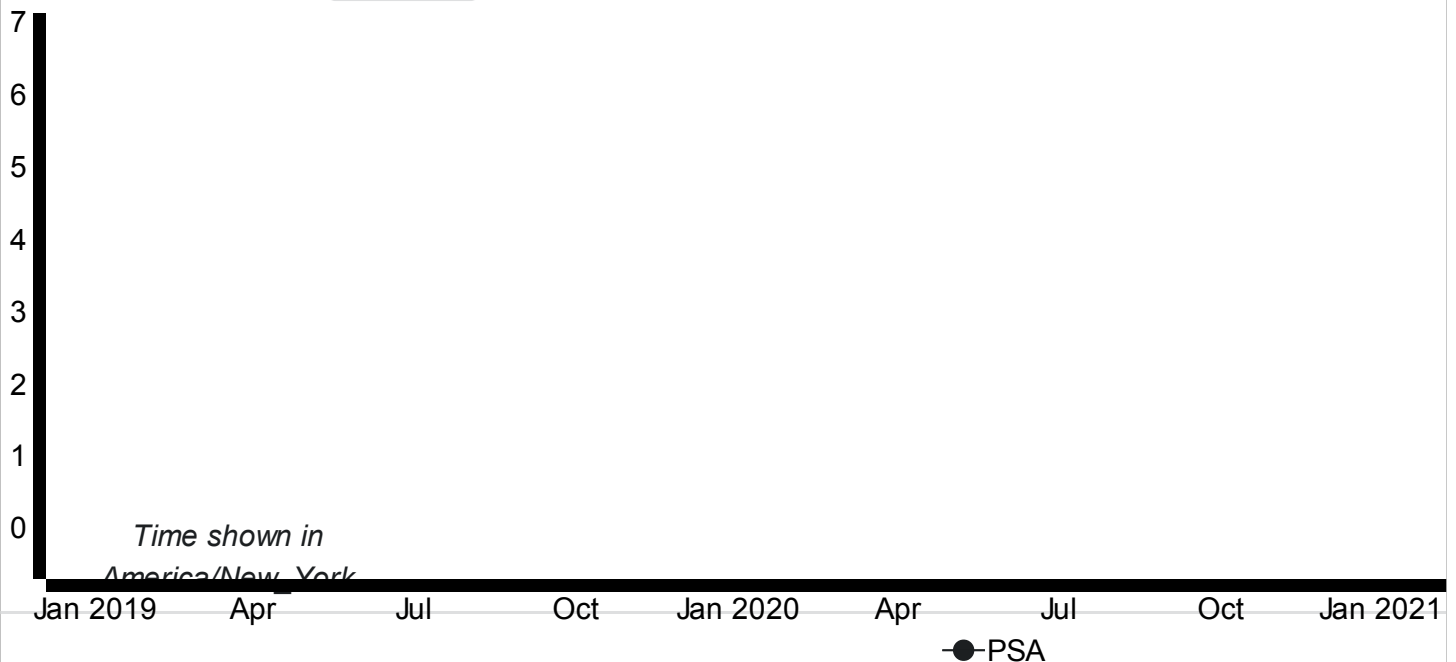

6.510 ng/mL (High)

Date: Dec 13, 2021 10:54 a.m. EST

Reference Range: 0.000 ng/mL - 4.000 ng/mL [Show less info](#)

Ordered By: Afridi , Salim K MD Dec 13, 2021 09:42 p.m. EST

Note: This test was performed on the Abbott ALINITY Instrument. Baselining with the Siemens assay is not offered due to a national shortage of reagents.

← Results

History

The information provided below is in the electronic medical record. If you believe any data is incorrect, please notify your healthcare provider.

GORDON WATTS

PSA (ng/mL)

Time Range

3 years ▼



Time shown in America/New_York.

6.510 ng/mL (High)

| | |
|-----------------------------|---------------------------|
| Date: | Reference |
| Dec 13, 2021 10:54 a.m. EST | Range: |
| | 0.000 ng/mL - 4.000 ng/mL |

Ordered By: Afridi , Salim K MD